


# RayBio® Human GITR ELISA Kit

**User Manual (for Cell Lysate and  
Tissue Lysate)**

**(Revised Mar 1, 2012)**

**RayBio® Human GITR ELISA  
Kit Protocol**

(Cat#: ELH-GITR-001C)



**RayBiotech, Inc.**

**We Provide You With Excellent  
Protein Array System And Service**

**Tel:(Toll Free)1-888-494-8555 or 770-729-2992; Fax:770-206-2393;  
Web: [www.raybiotech.com](http://www.raybiotech.com) Email: [info@raybiotech.com](mailto:info@raybiotech.com)**



RayBiotech, Inc.

---

**RayBio® Human GTR  
ELISA Kit Protocol**

**TABLE OF CONTENTS**

I.	Introduction.....	2
II.	Reagents.....	2
III.	Storage.....	3
IV.	Additional Materials Required.....	3
V.	Reagent Preparation.....	4
VI.	Assay Procedure.....	5
VII.	Assay Procedure Summary.....	7
VIII.	Calculation of Results	
A.	Typical Data.....	8
B.	Sensitivity.....	8
C.	Recovery.....	8
D.	Linearity.....	9
E.	Reproducibility.....	9
IX.	Specificity.....	9
X.	References.....	10
XI.	Troubleshooting Guide.....	11

## I. INTRODUCTION

GITR (glucocorticoid induced tumor necrosis factor receptor family related gene) is a type-1 transmembrane protein of 228 amino acids belonging to the TNF and NGF receptor family of proteins. GITR is expressed in normal T-lymphocytes from thymus, spleen. Constitutive expression of a transfected GITR gene induces resistance to apoptosis induced by anti CD3 monoclonal antibodies. The human homolog of GITR is expressed in lymph node and peripheral blood leukocytes. Its expression is up-regulated in human peripheral mononuclear cells mainly after stimulation with antibodies against CD3 and CD28.

The RayBio® Human GITR ELISA (Enzyme-Linked Immunosorbent Assay) kit is an in vitro enzyme-linked immunosorbent assay for the quantitative measurement of human GITR in cell lysate and tissue lysate. This assay employs an antibody specific for human GITR coated on a 96-well plate. Standards and samples are pipetted into the wells and GITR present in a sample is bound to the wells by the immobilized antibody. The wells are washed and biotinylated anti-human GITR antibody is added. After washing away unbound biotinylated antibody, HRP-conjugated streptavidin is pipetted to the wells. The wells are again washed, a TMB substrate solution is added to the wells and color develops in proportion to the amount of GITR bound. The Stop Solution changes the color from blue to yellow, and the intensity of the color is measured at 450 nm.

## II. REAGENTS

1. GITR Microplate (Item A): 96 wells (12 strips x 8 wells) coated with anti-human GITR.
2. Wash Buffer Concentrate (20x) (Item B): 25 ml of 20x concentrated solution.
3. Standards (Item C): 2 vials, recombinant human GITR.

4. Sample Diluent Buffer (Item D): 10 ml of 5x concentrated buffer. For Standard/Sample (cell lysate/tissue lysate) diluent.
5. Assay Diluent (Item E): 15 ml of 5x concentrated buffer. For Detection Antibody (Item F) and HRP-Streptavidin concentrate (Item G) diluent.
6. Detection Antibody GITR (Item F): 2 vial of biotinylated anti-human GITR (each vial is enough to assay half microplate).
7. HRP-Streptavidin concentrate (Item G): 200  $\mu$ l 400x concentrated HRP-conjugated streptavidin.
8. TMB One-Step Substrate Reagent (Item H): 12 ml of 3,3',5,5'-tetramethylbenzidine (TMB) in buffered solution.
9. Stop Solution (Item I): 8 ml of 0.2 M sulfuric acid.
10. Cell lysate buffer (Item J): 5 ml 2x cell lysate buffer.

### **III. STORAGE**

May be stored for up to 6 months at 2° to 8°C from the date of shipment. Standard (recombinant protein) should be stored at -20 °C or -80 °C (recommended at -80 °C) after reconstitution. Opened Microplate Wells or reagents may be store for up to 1 month at 2° to 8°C. Return unused wells to the pouch containing desiccant pack, reseal along entire edge.

Note: the kit can be used within one year if the whole kit is stored at -20 °C. Avoid repeated freeze-thaw cycles.


### **IV. ADDITIONAL MATERIALS REQUIRED**

- 1 Microplate reader capable of measuring absorbance at 450 nm.
- 2 Precision pipettes to deliver 2  $\mu$ l to 1 ml volumes.
- 3 Adjustable 1-25 ml pipettes for reagent preparation.
- 4 100 ml and 1 liter graduated cylinders.
- 5 Absorbent paper.
- 6 Distilled or deionized water.
- 7 Log-log graph paper or computer and software for ELISA data analysis.

8 Tubes to prepare standard or sample dilutions.

## V. REAGENT PREPARATION

1. Bring all reagents and samples to room temperature (18 - 25°C) before use.
2. Sample dilution: Tissue lysate and cell lysate sample should be diluted at least 5-fold with 1x Sample Diluent Buffer.
3. Sample Diluent Buffer/Assay Diluent should be diluted 5-fold with deionized or distilled water.
4. Preparation of standard: **Briefly spin the vial of Item C.** Add 400 µl 1x Sample Diluent Buffer (Item D) into Item C vial to prepare a 100 ng/ml standard. **Dissolve the powder thoroughly by a gentle mix.** Add 60 µl GITR standard from the vial of Item C, into a tube with 540 µl 1x Sample Diluent Buffer to prepare a 10,000 pg/ml stock standard solution. Pipette 400 µl 1x Sample Diluent Buffer into each tube. Use the stock standard solution to produce a dilution series (shown below). Mix each tube thoroughly before the next transfer. 1x Sample Diluent Buffer serves as the zero standard (0 pg/ml).

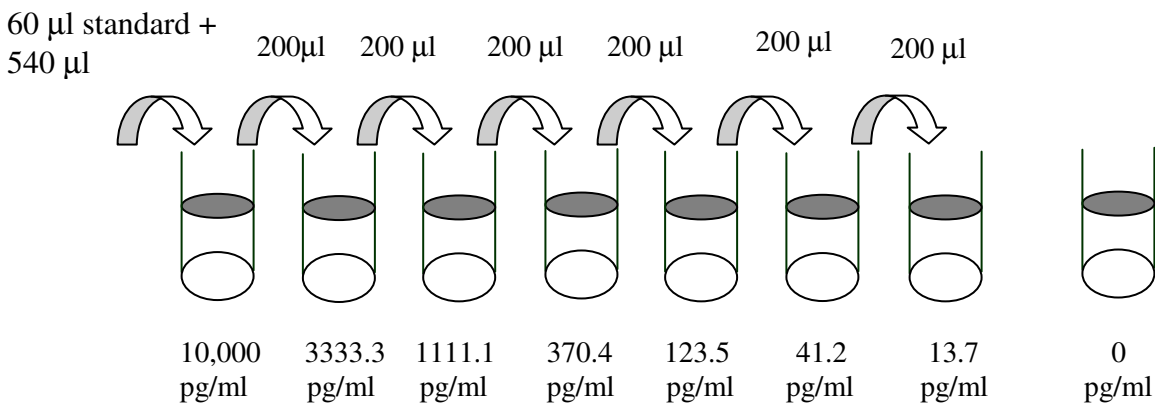

5. If the Wash Concentrate (20x) (Item B) contains visible crystals, warm to room temperature and mix gently until dissolved. Dilute 20 ml of Wash Buffer Concentrate into deionized or distilled water to yield 400 ml of 1x Wash Buffer.
6. Briefly spin the Detection Antibody vial (Item F) before use. Add 100  $\mu$ l of 1x Assay Diluent into the vial to prepare a detection antibody concentrate. Pipette up and down to mix gently (the concentrate can be stored at 4°C for 5 days). The detection antibody concentrate should be diluted 80-fold with 1x Assay Diluent and used in step 4 of Part VI Assay Procedure.
7. Briefly spin the HRP-Streptavidin concentrate vial (Item G) and pipette up and down to mix gently before use. HRP-Streptavidin concentrate should be diluted 400-fold with 1x Assay Diluent.

*For example: Briefly spin the vial (Item G) and pipette up and down to mix gently . Add 30  $\mu$ l of HRP-Streptavidin concentrate into a tube with 12 ml 1x Assay Diluent to prepare a 400-fold diluted HRP-Streptavidin solution (don't store the diluted solution for next day use). Mix well.*

8. Cell lysate buffer is diluted to 2-fold with deionized or distilled water (for cell lysate and tissue lysate).

## **VI. ASSAY PROCEDURE:**

1. Bring all reagents and samples to room temperature (18 - 25°C) before use. It is recommended that all standards and samples be run at least in duplicate.
2. Add 100  $\mu$ l of each standard (see Reagent Preparation step 2) and sample into appropriate wells. Cover well and incubate for 2.5 hours at room temperature or over night at 4°C with gentle shaking.

*We recommend using 50-500 µg/ml of total protein for lysate sample. The amount of sample used depends on the abundance of target protein. More of the sample can be used if signals are too weak. If signals are too strong, the sample can be diluted further.*

3. Discard the solution and wash 4 times with 1x Wash Solution. Wash by filling each well with Wash Buffer (300 µl) using a multi-channel Pipette or autowasher. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.
4. Add 100 µl of 1x prepared biotinylated antibody (Reagent Preparation step 6) to each well. Incubate for 1 hour at room temperature with gentle shaking.
5. Discard the solution. Repeat the wash as in step 3.
6. Add 100 µl of prepared Streptavidin solution (see Reagent Preparation step 7) to each well. Incubate for 45 minutes at room temperature with gentle shaking.
7. Discard the solution. Repeat the wash as in step 3.
8. Add 100 µl of TMB One-Step Substrate Reagent (Item H) to each well. Incubate for 30 minutes at room temperature in the dark with gentle shaking.
9. Add 50 µl of Stop Solution (Item I) to each well. Read at 450 nm immediately.

## **VII. ASSAY PROCEDURE SUMMARY**

1. Prepare all reagents, samples and standards as instructed.  
↓
2. Add 100 µl standard or sample to each well.  
Incubate 2.5 hours at room temperature or over night at 4°C.  
↓
3. Add 100 µl prepared biotin antibody to each well.  
Incubate 1 hour at room temperature.  
↓
4. Add 100 µl prepared Streptavidin solution.  
Incubate 45 minutes at room temperature.  
↓
5. Add 100 µl TMB One-Step Substrate Reagent to each well.  
Incubate 30 minutes at room temperature.  
↓
6. Add 50 µl Stop Solution to each well.  
Read at 450 nm immediately.


## **VIII. CALCULATION OF RESULTS**

Calculate the mean absorbance for each set of duplicate standards, controls and samples, and subtract the average zero standard optical density. Plot the standard curve on log-log graph paper or using Sigma plot software, with standard concentration on the x-axis and absorbance on the y-axis. Draw the best-fit straight line through the standard points.



## A. TYPICAL DATA

These standard curves are for demonstration only. A standard curve must be run with each assay.

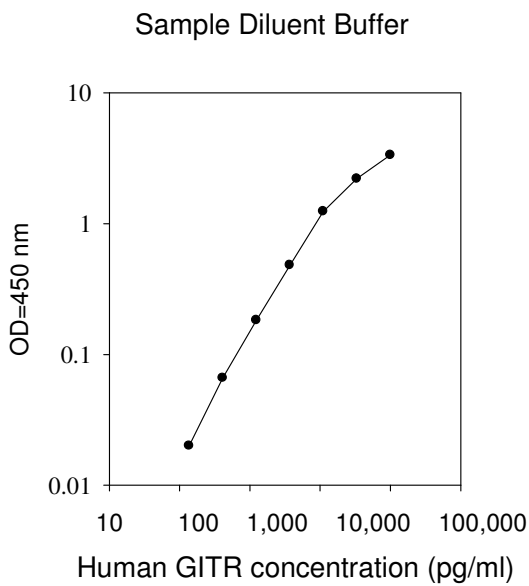

## B. SENSITIVITY

The minimum detectable dose of GITR is typically less than 15 pg/ml.

## C. RECOVERY

Recovery was determined by spiking various levels of human GITR into human tissue lysate and cell lysate. Mean recoveries are as follows:

Sample Type	Average % Recovery	Range (%)
Tissue lysate	94.92	82-102
Cell lysate	93.49	83-103

## D. LINEARITY

---

Sample Type	Tissue Lysate	Cell lysate
1:2 Average % of Expected Range (%)	88 82-102	87 83-103
1:4 Average % of Expected Range (%)	93 84-103	94 85-104

---

## E. REPRODUCIBILITY

Intra-Assay: CV<10%

Inter-Assay: CV<12%

## IX. SPECIFICITY

Cross Reactivity: This ELISA kit shows no cross-reactivity with any of the cytokines tested (*e.g.*, human Angiogenin, BDNF, BLC, ENA-78, FGF-4, IL-1 $\alpha$ , IL-1 $\beta$ , IL-2, IL-3, IL-4, IL-5, IL-7, IL-8, IL-9, IL-10, IL-11, IL-12 p70, IL-12 p40, IL-13, IL-15, IL-309, IP-10, G-CSF, GM-CSF, IFN- $\gamma$ , Leptin, MCP-1, MCP-2, MCP-3, MDC, MIP-1 $\alpha$ , MIP-1  $\beta$ , MIP-1 $\delta$ , PARC, PDGF, RANTES, SCF, TARC, TGF- $\beta$ , TIMP-1, TIMP-2, TNF- $\alpha$ , TNF- $\beta$ , TPO, VEGF).

## **X. REFERENCES:**

1. **Gurney AL et al.** Identification of a new member of the tumor necrosis factor family and its receptor, a human ortholog of mouse GITR. *Current Biology* 9(4): 215-8 (1999).
2. **Kwon B et al.** Identification of a novel activation-inducible protein of the tumor necrosis factor receptor superfamily and its ligand. *Journal of Biological Chemistry* 274(10): 6056-61 (1999).
3. **Nocentini G et al.** A new member of the tumor necrosis factor nerve growth factor receptor family inhibits t cell receptor induced apoptosis. *Proceedings of the National Academy of Science (USA)* 94(12): 6216-6221 (1997).

## XI. TROUBLESHOOTING GUIDE

<b>Problem</b>	<b>Cause</b>	<b>Solution</b>
1. Poor standard curve	<ol style="list-style-type: none"> <li>1. Inaccurate pipetting</li> <li>2. Improper standard dilution</li> </ol>	<ol style="list-style-type: none"> <li>1. Check pipettes</li> <li>2. Ensure briefly spin the vial of Item C and dissolve the powder thoroughly by a gentle mix.</li> </ol>
2. Low signal	<ol style="list-style-type: none"> <li>1. Too brief incubation times</li> <li>2. Inadequate reagent volumes or improper dilution</li> </ol>	<ol style="list-style-type: none"> <li>1. Ensure sufficient incubation time; assay procedure step 2 change to over night</li> <li>2. Check pipettes and ensure correct preparation</li> </ol>
3. Large CV	<ol style="list-style-type: none"> <li>1. Inaccurate pipetting</li> </ol>	<ol style="list-style-type: none"> <li>1. Check pipettes</li> </ol>
4. High background	<ol style="list-style-type: none"> <li>1. Plate is insufficiently washed</li> <li>2. Contaminated wash buffer</li> </ol>	<ol style="list-style-type: none"> <li>1. Review the manual for proper wash. If using an a plate washer, check that all ports are unobstructed.</li> <li>2. Make fresh wash buffer</li> </ol>
5. Low sensitivity	<ol style="list-style-type: none"> <li>1. Improper storage of the ELISA kit</li> <li>2. Stop solution</li> </ol>	<ol style="list-style-type: none"> <li>1. Store your standard at <math>&lt;-20^{\circ}\text{C}</math> after reconstitution, others at <math>4^{\circ}\text{C}</math>. Keep substrate solution protected from light</li> <li>2. Stop solution should be added to each well before measure</li> </ol>

RayBio® ELISA kits:

Over 200 ELISA kits, custom ELISA kit choose from over 500 list visit [www.raybiotech.com](http://www.raybiotech.com) for details.

This product is for research use only.



©2004 RayBiotech, Inc.