

Free Glycerol Assay Kit

(Catalog #K630-100; 100 assays; Store at -20°C)

I. Introduction:

Glycerol is widely used in foods, beverages, solvents, pharmaceutical and cosmetic products, etc. There is broad interest in quantification of glycerol for research and development. BioVision's Glycerol Assay Kit provides a sensitive, easy assay to measure free glycerol concentration in various samples. In the assay, glycerol is enzymatically oxidized to generate a product which reacts with the probe to generate color ($\lambda = 570$ nm) and fluorescence (Ex/Em = 535/587 nm). The kit can detect 50 pmol-10 nmol (or 1-10000 μ M range) of glycerol in various samples.

II. Kit Contents:

Components	K630-100	Cap Code	Part Number
Glycerol Assay Buffer	25 ml	WM	K630-100-1
Glycerol Probe (in DMSO, Anhydrous)	0.2 ml	Red	K630-100-2A
Glycerol Enzyme Mix (lyophilized)	1 vial	Green	K630-100-4
Glycerol Standard (100 mM)	0.2 ml	Yellow	K630-100-5

III. Storage and Handling:

Store kit at -20°C, protected from light. Warm Assay Buffer to room temperature before use. Briefly centrifuge all small vials prior to opening.

IV. Reagents Preparation and Storage Conditions:

Glycerol Enzyme Mix: Dissolve in 220 μ l Assay Buffer. Aliquot and store at -20°C. Use within two months.

Glycerol Probe: Briefly warm at 37°C for 1-2 min to dissolve. Mix well. Store at -20°C. Use within two months.

V. Glycerol Assay Protocol:

1. Standard Curve Preparation:

For the colorimetric assay, add 10 μ l of the glycerol standard to 990 μ l of Assay Buffer to generate 1 mM glycerol standard, mix well. Add 0, 2, 4, 6, 8, 10 μ l into each well individually. Adjust volume to 50 μ l/well with Assay Buffer to generate 0, 2, 4, 6, 8, 10 nmol/well of glycerol Standard.

For the fluorometric assay, dilute the Glycerol Standard to 0.01- 0.1 mM with the Assay Buffer (Detection sensitivity is 10-100 fold higher for a fluorometric than a colorimetric assay). Follow the protocol as for the colorimetric assay.

2. Sample Preparation: Prepare test samples to a final volume of 50 μ l/well with Assay Buffer in a 96-well plate. We suggest testing several dilutions of your sample to make sure the readings are within the standard curve range.

3. Reaction Mix: Mix enough reagent for the number of samples and standards to be performed: For each well, prepare a total 50 μ l Reaction Mix:

- 46 μ l Assay Buffer
- 2 μ l Glycerol Probe
- 2 μ l Glycerol Enzyme Mix

4. Add 50 μ l of the Reaction Mix to each well containing standard and samples. Mix well. Incubate at room temperature for 30 min, protect from light.

5. Measure OD 570 nm for the colorimetric assay or Ex/Em = 535/590 nm for the fluorometric assay in a microtiter plate reader. The reaction is stable for at least two hrs.


6. Calculations: Correct background by subtracting the value derived from the 0 glycerol standard from all sample readings. Plot the standard curve (OD 570nm or Fluorescence readings vs. nmol). Apply sample readings to the standard curve. Glycerol concentration can then be calculated:

$$C = Ga / Sv \text{ nmol}/\mu\text{l or } \mu\text{mol}/\text{ml or mM}$$

Where: **Ga** is Glycerol amount from standard curve (nmol).

Sv is the sample volume (before dilution) added in sample wells (μ l).

Glycerol molecular weight: 92.09.

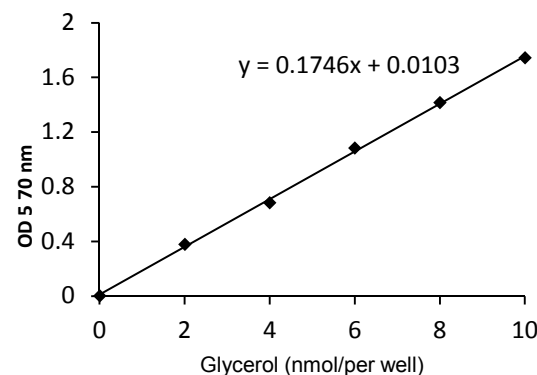

RELATED PRODUCTS:

- | | |
|---------------------------------|--|
| NAD/NADH Quantification Kit | NADP/NADPH Quantification Kit |
| ADP/ATP Ratio Assay Kit | Ascorbic Acid Quantification Kit |
| Glucose Assay Kit | Fatty Acid Assay Kit |
| Ethanol Assay Kit | Uric Acid Assay Kit |
| Pyruvate Assay Kit | Lactate Assay Kit/ II |
| Creatine Assay Kit | Creatinine Assay Kit |
| Ammonia Assay Kit | Free Glycerol Assay Kit |
| Triglyceride Assay Kit | Hemin Assay Kit |
| Choline/Acetylcholine Assay Kit | Total Antioxidant Capacity (TAC) Assay Kit |
| Sarcosine Assay Kit | L-Amino Acid Assay Kit |
| Nitric Oxide Assay Kit | Glutathione Detection Kit s |
| ADP & ATP Colorimetric Kits | ADP & ATP fluorometric Kits |
| Glutamate Assay Kit | Glycerol Assay Kit |
| Cholesterol Assay Kit | HDL & LDL/VLDL Assay Kits |
| Starch Assay Kit | Glycogen Assay Kit |
| NAD/NADH Assay Kit | NADP/NADPH Assay Kit |
| Heme Assay Kit | Ascorbic Acid Assay Kit |
| Calcium Assay Kit | Iron Assay Kit |

FOR RESEARCH USE ONLY! Not to be used on humans.

GENERAL TROUBLESHOOTING GUIDE:

Problems	Cause	Solution
Assay not working	<ul style="list-style-type: none"> • Use of ice-cold assay buffer • Omission of a step in the protocol • Plate read at incorrect wavelength • Use of a different 96-well plate 	<ul style="list-style-type: none"> • Assay buffer must be at room temperature • Refer and follow the data sheet precisely • Check the wavelength in the data sheet and the filter settings of the instrument • Fluorescence: Black plates (clear bottoms) ; Luminescence: White plates ; Colorimeters: Clear plates
Samples with erratic readings	<ul style="list-style-type: none"> • Use of an incompatible sample type • Samples prepared in a different buffer • Samples were not deproteinized (if indicated in datasheet) • Cell/ tissue samples were not completely homogenized • Samples used after multiple free-thaw cycles • Presence of interfering substance in the sample • Use of old or inappropriately stored samples 	<ul style="list-style-type: none"> • Refer data sheet for details about incompatible samples • Use the assay buffer provided in the kit or refer data sheet for instructions • Use the 10 kDa spin cut-off filter or PCA precipitation as indicated • Use Dounce homogenizer (increase the number of strokes); observe for lysis under microscope • Aliquot and freeze samples if needed to use multiple times • Troubleshoot if needed, deproteinize samples • Use fresh samples or store at correct temperatures till use
Lower/ Higher readings in Samples and Standards	<ul style="list-style-type: none"> • Improperly thawed components • Use of expired kit or improperly stored reagents • Allowing the reagents to sit for extended times on ice • Incorrect incubation times or temperatures • Incorrect volumes used 	<ul style="list-style-type: none"> • Thaw all components completely and mix gently before use • Always check the expiry date and store the components appropriately • Always thaw and prepare fresh reaction mix before use • Refer datasheet & verify correct incubation times and temperatures • Use calibrated pipettes and aliquot correctly
Readings do not follow a linear pattern for Standard curve	<ul style="list-style-type: none"> • Use of partially thawed components • Pipetting errors in the standard • Pipetting errors in the reaction mix • Air bubbles formed in well • Standard stock is at an incorrect concentration • Calculation errors • Substituting reagents from older kits/ lots 	<ul style="list-style-type: none"> • Thaw and resuspend all components before preparing the reaction mix • Avoid pipetting small volumes • Prepare a master reaction mix whenever possible • Pipette gently against the wall of the tubes • Always refer the dilutions in the data sheet • Recheck calculations after referring the data sheet • Use fresh components from the same kit
Unanticipated results	<ul style="list-style-type: none"> • Measured at incorrect wavelength • Samples contain interfering substances • Use of incompatible sample type • Sample readings above/below the linear range 	<ul style="list-style-type: none"> • Check the equipment and the filter setting • Troubleshoot if it interferes with the kit • Refer data sheet to check if sample is compatible with the kit or optimization is needed • Concentrate/ Dilute sample so as to be in the linear range
<p>Note: The most probable list of causes is under each problem section. Causes/ Solutions may overlap with other problems.</p>		